

Botany Evolution LLC

2510 Kirby Circle NE
Palm Bay, FL 32945
321-802-4583

Certificate Of Analysis

Sample Identification Information

Date of Analysis 3/6/2018
Sample: S0364
Product Name CEREMONIAL
Lot# VFE180212C

Country of Origin/Region VANUATU
Country of Processing VANUATU
Manufacture Date 02/12/18
Expiration Date 02/12/21

General Product Specifications

Product Species Piper Methysticum
Part Used Root

Common Names Kava kava, Awa, Yagona
Appearance Beige powder

Analyzed Characteristics

Specification

Result

Test Method

<u>Standardization</u>	2-15% Kavalactones	9.70%	HPLC
<u>Identification</u>	Complies by HPLC	Conform	HPLC
<u>Kavalactone Profile</u>	Noble	PASS	HPLC
<u>Mesh Size</u>	60-30	60	Sieve
<u>Color</u>	Beige to Yellow	Pass	Visual
<u>Odor</u>		Pass	Organoleptic
<u>Taste</u>		Pass	Organoleptic
<u>Chemotype</u>		243156	HPLC
<u>K/DHM</u>		3.57	Calculation

Kavalactones	Code	Peaks Ref.	Correction Factor	Area *	Area %	Corrected Kavalactones	Chemotype Identifier
Standard Kavain	K			3009.651			
Methysticin	M	1	2.19	711.746	6.87%	0.74%	6
Dihydromethysticin	DHM	2	3.23	520.857	5.03%	0.80%	5
Kavain	K	3	1	6005.186	57.99%	2.85%	4
Dihydrokavain	DHK	4	4.21	1567.451	15.14%	3.13%	2
Desmethoxyyangonin	DMY	5	2.74	665.473	6.43%	0.86%	1
Yangonin	Y	6	3.16	884.226	8.54%	1.32%	3
Kavalactones			Total:	10354.939	100.00%	9.70%	243156

*See data in attachment HPLC1100 Agilent Certificate with Chromatogram graph.

This result are in house tested and the best of our knowledge and experience. Using calibrated equipment.
We are dedicated to offer the best Quality of Botanical products on the market. We test and stand behind our products.
Disclaimer* the test results are accurate to the best of our knowledge and are based upon reputable laboratory and industry standard testing methods.
These results should not be used as a final determination for use in a finished product. It is recommended that you verify these test results with an in house quality control department or obtain an additional independent third party lab to verify that this material meets specifications
Botany Evolution, its board of directors, contract laboratories, employees, and affiliates are held harmless from any loss or damages resulting from the use or misuse of this document. The appropriate use of this product is the sole responsibility of the user of the purchasing party.

Muste Youngs 3/8/18

SAMPLE S0364
Vial 14

0.75022g/50ml

wavelength 246 nm

C:\CHEM32\1\DATA\KAVA_3_6_2018_15MINSTDTESTMETHOD 2018-03-06 14-56-18\014-->

SEQUENCE C:\CHEM32\1\DATA\KAVA_3_6_2018_ ->


Injection date 3/6/2018

Injection time 7:47:31 PM

Acq. operator KRISTL

Method C:\CHEM32\1\METHODS\KAVA15MIN_STD_TEST.M

DAD1 C, Sig=246,10 Ref=500,60 (KAVA_3_6_2018_15MINSTDTESTMETHOD 2018-03-06 14-56-18\014-1501.D)

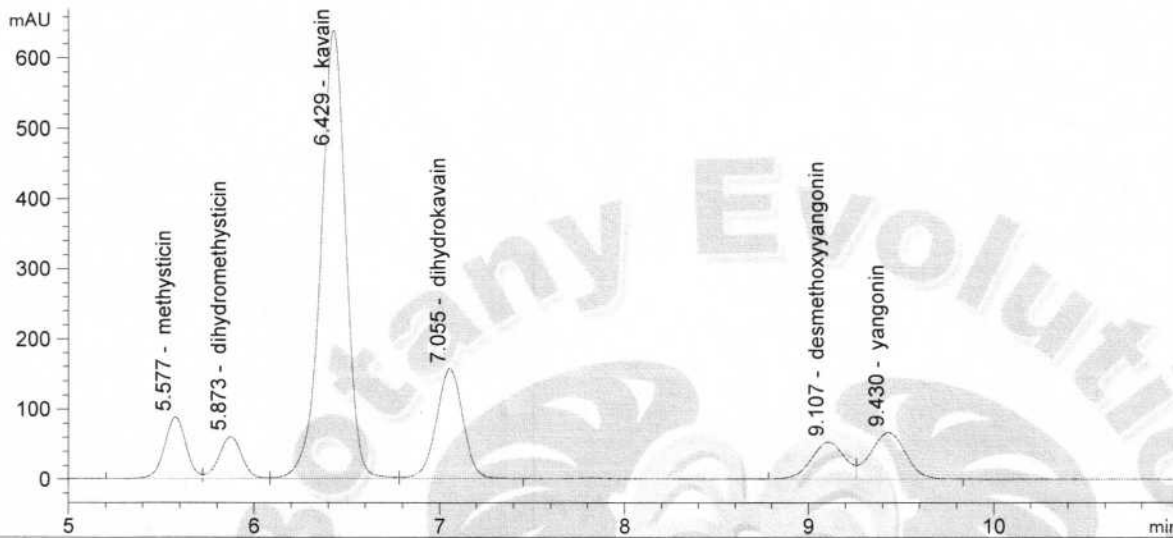

#	COMPOUND	RET. TIME	AREA	AREA %	AMOUNT
1	methysticin	5.577	711.746	6.87	0.000
2	dihydromethysticin	5.873	520.857	5.03	0.000
3	kavain	6.429	6005.186	57.99	0.000
4	dihydrokavain	7.055	1567.451	15.14	0.001
5	desmethoxyyangonin	9.107	665.473	6.43	0.000
6	yangonin	9.430	884.226	8.54	0.000

3/8/18
VJ